



## SHIMADZU NEXIS GC-2030

Clarity Control Module

ENG

Code/Rev.: M240/80D  
Date: 3/14/2022

Phone: +420 251 013 400  
Fax: +420 251 013 401  
clarity@dataapex.com  
www.dataapex.com

DataApex Ltd.  
Petrzilkova 2583/13  
158 00 Prague 5  
The Czech Republic

Clarity<sup>®</sup>, DataApex<sup>®</sup> and ▲<sup>®</sup> are trademarks of DataApex Ltd. Microsoft<sup>®</sup> and Windows<sup>™</sup> are trademarks of Microsoft Corporation.

*DataApex reserves the right to make changes to manuals without prior notice. Updated manuals can be downloaded from [www.dataapex.com](http://www.dataapex.com).*

Author: MT

# Contents

<b>1 Shimadzu Nexis GC-2030</b> .....	<b>1</b>
<b>2 Requirements</b> .....	<b>2</b>
2.1 Software requirements .....	2
2.2 Hardware requirements .....	2
<b>3 Installation procedure</b> .....	<b>3</b>
3.1 Installing Correct Version of ICF .....	3
3.2 Network connections .....	4
3.3 Clarity - Shimadzu Edition Configuration .....	5
3.4 Installation Qualification of Shimadzu Nexis GC-2030 .....	9
<b>4 Using the Shimadzu Nexis GC-2030</b> .....	<b>11</b>
4.1 Method Setup - GC .....	11
4.2 Device Monitor .....	15
<b>5 Troubleshooting</b> .....	<b>16</b>
5.1 Specific Problems .....	17

To facilitate the orientation in the **Shimadzu Nexis GC-2030** manual and **Clarity - Shimadzu Edition** chromatography station, different fonts are used throughout the manual. Meanings of these fonts are:

**Instrument** (blue text) marks the name of the window to which the text refers.

*Open File* (italics) describes the commands and names of fields in **Clarity - Shimadzu Edition**, parameters that can be entered into them or a window or dialog name (when you already are in the topic describing the window).

WORK1 (capitals) indicates the name of the file and/or directory.

*ACTIVE* (capital italics) marks the state of the station or its part.

The bold text is sometimes also used for important parts of the text and the name of the **Clarity - Shimadzu Edition** station. Moreover, some sections are written in format other than normal text. These sections are formatted as follows:

---

**Note:** Notifies the reader of relevant information.

---

**Caution:** Warns the user of possibly dangerous or very important information.

---

**■ Marks the problem statement or trouble question.**

**Description:** Presents more detailed information on the problem, describes its causes, etc.

**Solution:** Marks the response to the question, presents a procedure how to remove it.

# 1 Shimadzu Nexis GC-2030

This manual describes the use of the **Shimadzu Nexis GC-2030** with the **Clarity - Shimadzu Edition** software.



*Fig 1: Shimadzu Nexis GC-2030*

**Shimadzu Nexis GC-2030** is controlled using RC.NET driver developed by **Shimadzu** running under the Agilent ICF (Instrument Control Framework) library developed by Agilent, which can be run within the **Clarity - Shimadzu Edition** environment.

## 2 Requirements

### 2.1 Software requirements

**Shimadzu Nexis GC-2030** requires for correct installation and **Microsoft .NET version 4.7.2** or higher for operation. Both of the versions are already installed on majority of PCs. Nonetheless you will be notified during the installation if your PC is missing any version of **Microsoft .NET** - then follow the instructions there.

Required operating systems:

- **Windows 7 SP1 (32/64 bit)**
- **Windows 8.1 (32/64 bit)**
- **Windows 10 (32/64 bit)**
- **Windows 11 (only 64 bit)**

For complete list of .NET requirements, see the **.NET Framework System Requirements** on Microsoft web page.

---

**Caution:** Before installing **Clarity - Shimadzu Edition**, make sure that your **Windows** are updated to the latest version.

### 2.2 Hardware requirements

- LAN interface installed on PC is required.
- Latest available firmware version (**minimal version is 1.09**) of the module should be used to ensure maximum compatibility.

For complete list of supported Windows OS, instrument firmware, see Shimadzu webpages.

## 3 Installation procedure

**Shimadzu Nexis GC-2030** is part of the **Clarity - Shimadzu Edition** *Typical* installation. To install it, select the *Typical* installation or check the **Shimadzu GC2030** in the **Choose Components** dialog in *Instrument Control Framework (ICF)* during the installation of **Clarity - Shimadzu Edition**.

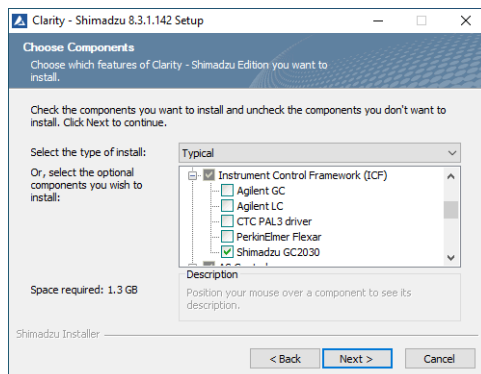


Fig 2: Typical installation of Clarity - Shimadzu Edition

### 3.1 Installing Correct Version of ICF

Clarity - Shimadzu Edition expects a specific version of Agilent ICF. Because other programs may also be using Agilent ICF, it is possible they've installed a different version than is supported by Clarity - Shimadzu Edition. In that case in the installation you will be prompted to reinstall it in order to install correct version. Going forward with this step is crucial for correct functionality of **Clarity - Shimadzu Edition** and **Shimadzu Nexis GC-2030**.

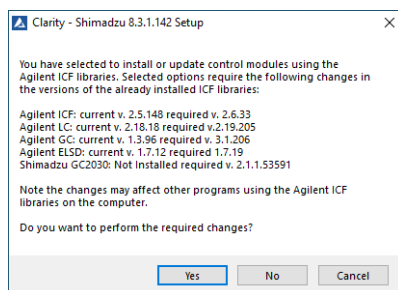


Fig 3: Installing correct version of Agilent ICF

**Note:** This reinstallation of Agilent ICF may cause that other programs using it, may not function properly.

## 3.2 Network connections

The instrument **Shimadzu Nexis GC-2030** has to be connected to a site network by LAN. It is recommended to attach the hardware directly to the PC avoiding hubs, switches etc. Always contact your local LAN administrator who can make the appropriate settings.

---

**Caution:** **Cross LAN** cable is primarily used for the direct connection of the instrument and the PC. This cable can also be used for the connection of the device to the switch or network socket, but with older switches, the **straight LAN** cable might be necessary.

### LAN Settings

PC: LAN card, TCP/IP protocol.

Both PC and **Shimadzu Nexis GC-2030** should be configured on the same IP range.

### Firewall

Ensure that the firewall does not block communication from the **Shimadzu Nexis GC-2030**.



### 3.3 Clarity - Shimadzu Edition Configuration

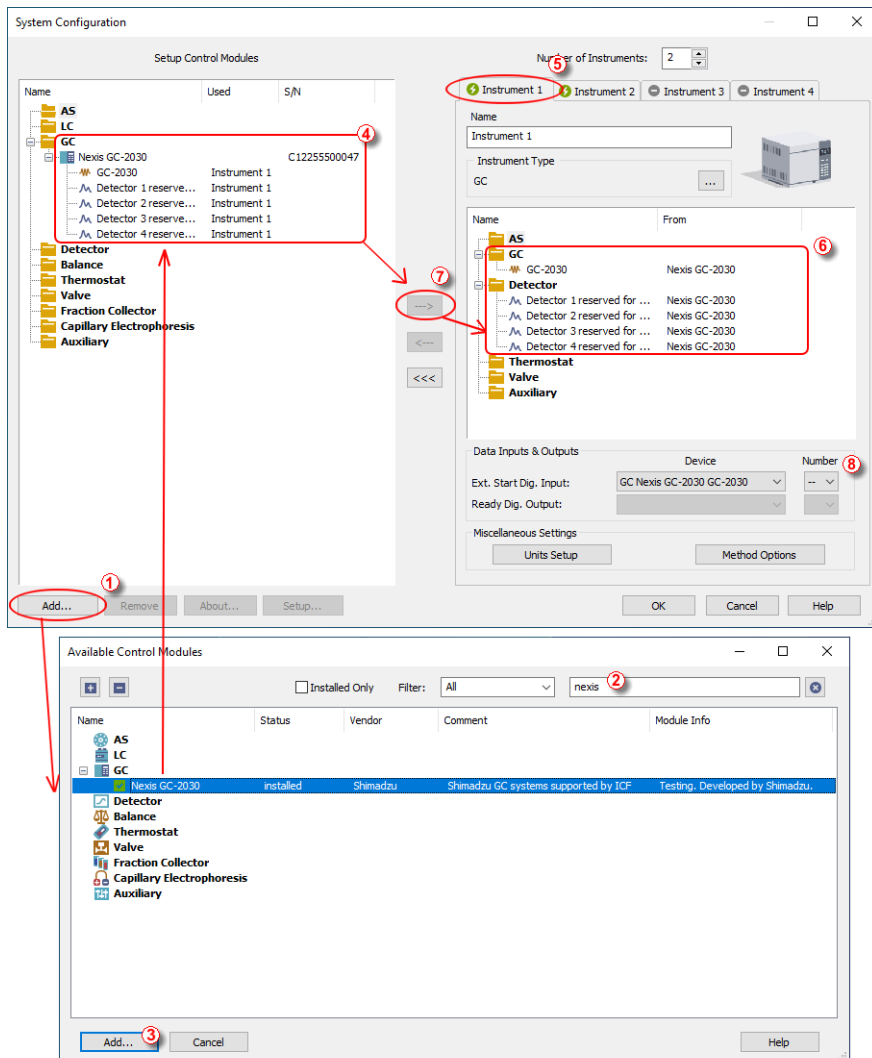


Fig 4: System Configuration

- Start the **Clarity - Shimadzu Edition** station by clicking on the  icon on the desktop.

- Open the [System Configuration](#) dialog accessible from the [Clarity - Shimadzu Edition](#) window using the *System - Configuration...* command.
- Press the *Add* button ① (See [3.3](#) on pg [5](#).) to invoke the [Available Control Modules](#) dialog.
- You can specify the searching filter ② to simplify the finding of the driver.
- Select the **Shimadzu Nexis GC-2030** item and press the *Add* ③ button. The [Nexis GC-2030 Setup](#) dialog will open.

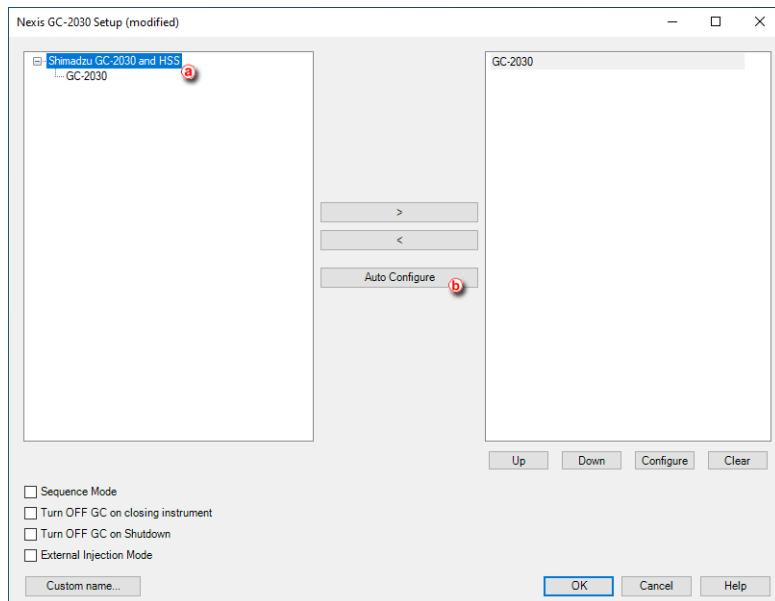


Fig 5: Nexis GC-2030 Setup

**Caution:** The *Sequence Mode* enables autosampler to prepare next sample during previous run (sequence will lock one row ahead). For correct operation in the *Sequence Mode* there have to be set corresponding parameters (Enable Sample Overlap) in the [ICF GC Method Setup](#) dialog (GC tab, section ALS, item Tray/Other).

**Note:** The *Turn OFF GC on closing instrument* and *Turn OFF GC on Shutdown* checkboxes govern the behavior of the GC while the *Instrument* window is closed and when *Shutdown* event is invoked (by user, by error or as a reaction from *Event Table*). When the function is not checked Clarity - Shimadzu Edition will not be able to shut down the Shimadzu Nexis GC-2030.

**Note:** The *Custom name...* button can be used to alter the name of the module. This change propagates to the module name in the *Setup Control Modules* ④ and in the *Data Inputs & Outputs* ⑧ sections of the *System Configuration* dialog. Default name is used when the field is left empty.

- Select appropriate instrument type ① and use Auto Configure ② button to open *Automatic Configuration parameters* dialog.

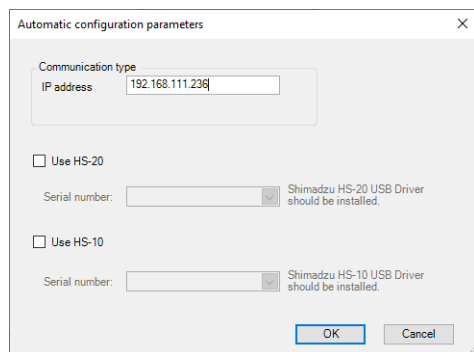




Fig 6: Automatic configuration parameters dialog

- Insert the *IP address* of Shimadzu Nexis GC-2030 and confirm. The address can be found or set using instrument's touch panel.
- Then click *OK* button in the lower part of the *Nexis CG-2030 Setup* dialog and the instrument will then appear in *System Configuration*, including all modules of the instrument (detector, autosampler etc.).

**Caution:** If you change the configuration of the **Nexis CG-2030** system (for example remove and add another instruments), the communication parameters like *IP address* will be lost and it is necessary to set them again.

- After previous steps drag and drop the **Nexis GC-2030** icon from the *Setup Control Modules* list ④ on the left side of the *System Configuration* dialog to the desired *Instrument* ⑤ tab on the right side ⑥ (or use the  button ⑦ to do so).
- Set the *Ext. Start Dig. Input* ⑧ on the right bottom side of the *System Configuration* dialog if you wish synchronize **Clarity - Shimadzu Edition** with **Shimadzu Nexis GC-2030** instrument over LAN. If the settings of the *Ext. Start Dig. Input* is set to default value  ⑧ the analysis start will be detected by **Clarity - Shimadzu Edition** by receiving data from the **Shimadzu Nexis GC-2030** configured detector on this **Shimadzu Nexis GC-2030 Instrument**. If this **Shimadzu Nexis GC-2030 Instrument** has no detector configured then it is necessary to set *Ext. Start Dig. Input* value

- ▾ ⑧ to value "1" - ▾ ⑧ to assure correctly synchronized start of the analysis with the **Shimadzu Nexis GC-2030** autosampler's injection.
- More detailed configuration parameters can be opened by using **Configure** button in **Nexis GC-2030 Setup**. In **Configure GC-2030** window double click on specific module. More settings can be set in opened window, specific to the module. For more detailed description of individual setting and parametrs press **F1** or **Help** button to open **Nexis GC-2030 help**.

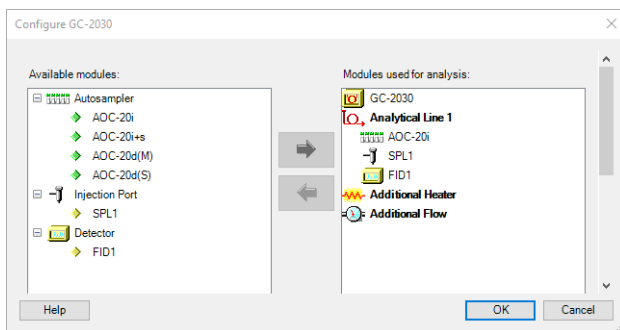


Fig 7: Configure GC-2030 dialog

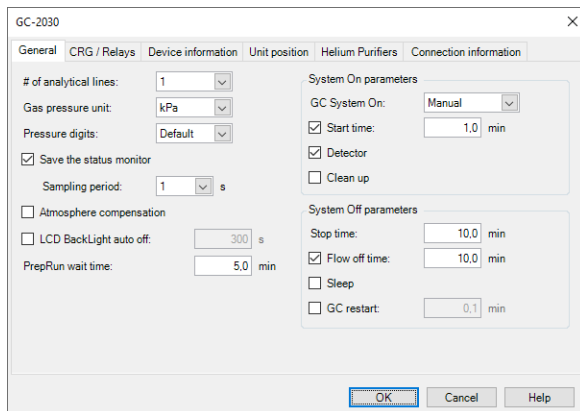


Fig 8: Module configuration dialog

**Note:** Press the **F1** key to display the **Nexis CG-2030 help** with detailed description of the dialog.

**Note:** The configuration dialog of the **Shimadzu Nexis CG-2030** subcomponents (detector/s, inlet...) can be displayed any time by double-clicking on its icon.

### 3.4 Installation Qualification of Shimadzu Nexis GC-2030

**Shimadzu Nexis GC-2030** is controlled via **Agilent ICF**, an external program developed by Agilent, and for that reason it must be validated using their utility. If you have installed Clarity - Shimadzu Edition with Agilent ICF, **the IQ is valid only if successful validation of ICF is attached.**

The validation of ICF can be performed directly from the [IQ Report](#).

**Caution:** When Clarity - Shimadzu Edition expects *Agilent ICF* is installed then **IQ** expects the same. If (due to any reason) the *Agilent ICF* installation is not found within Clarity - Shimadzu Edition, the *Installation Qualification Test* status is set by default to *FAILED*. To resolve this, it is necessary to re-install **Agilent ICF** through Clarity - Shimadzu Edition reinstallation and then perform **IQ** again.

Installation Qualification Report	
Date	12.08.2020, 12:02
Serial number of application	088-000888+40959/02
User Code	
Version of application	ClarityShimadzu version 8.3.1.142
Build date of application	07.08.2020, 14:54
Instruments	2
Extensions	SST; GPC; PDA; EA; CE; MS; NGA; DHA; SimDis; GCxGC; MS-TOF
Controls	GC; LC; AS
Certification file	C:\ClarityShimadzu-test\Biniq.chk
Checksum of cert. file	43E3CCCEBA47AB790
Date of cert. file	07.08.2020, 16:00
User	mirosalvt
System	Microsoft Windows 10 Professional version 10.0 (Build 18363)
Acquisition and hardware devices	Key Rockey 4ND 088-00888+40959/002 id:31EA3AEF Nexis GC-2030 C12255500047

**Core Files, Embedded Components: Passed**

**Files**

[Show files list >](#)

**3<sup>rd</sup> Party Packages**


**Agilent ICF:** .....

⚠ Agilent ICF is present in your system. It is necessary to perform its validation separately [here](#) ①  
The result must be attached to this report.

Fig 9: IQ Report with ICF installation present

Press the link "here" ① and then click the *Run* button to generate report. Several reports may be generated, depending on the number of ICF drivers you have installed. Reports will be automatically opened in the in your default internet browser.

Address field of the generated report displays the location of the actual report ②.

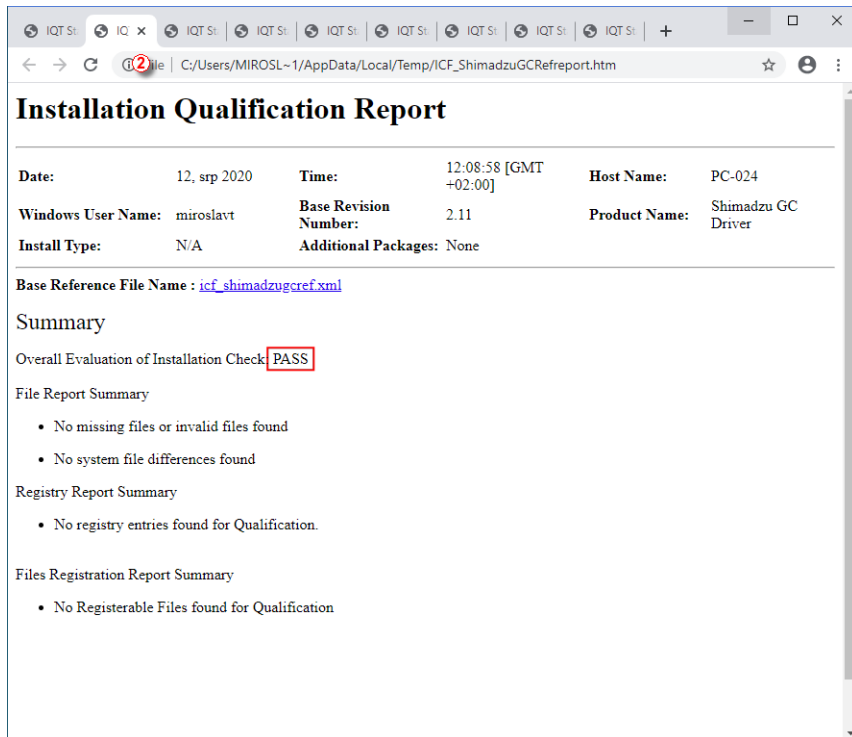

The screenshot shows a web browser window with the address bar containing the file path: C:/Users/MIROSL~1/AppData/Local/Temp/ICF\_ShimadzuGCRefreport.htm. The page title is "Installation Qualification Report".

<b>Date:</b>	12, srp 2020	<b>Time:</b>	12:08:58 [GMT +02:00]	<b>Host Name:</b>	PC-024
<b>Windows User Name:</b>	miroslavt	<b>Base Revision Number:</b>	2.11	<b>Product Name:</b>	Shimadzu GC Driver
<b>Install Type:</b>	N/A	<b>Additional Packages:</b>	None		

Base Reference File Name : [icf\\_shimadzugceref.xml](#)

### Summary

Overall Evaluation of Installation Check: **PASS**

File Report Summary

- No missing files or invalid files found
- No system file differences found

Registry Report Summary

- No registry entries found for Qualification.

Files Registration Report Summary

- No Registerable Files found for Qualification

Fig 10: ICF Report - PASS

## 4 Using the Shimadzu Nexis GC-2030

There are multiple places for setting the parameters of the **Shimadzu Nexis GC-2030** in the **Clarity - Shimadzu Edition**:

- the **Method Setup - GC tab**

**Caution:** Before opening the **Instrument** window with configured **Shimadzu Nexis GC-2030** device, ensure there is not any other PC connected to GC. Otherwise there will be raised an error during the connection.

### 4.1 Method Setup - GC

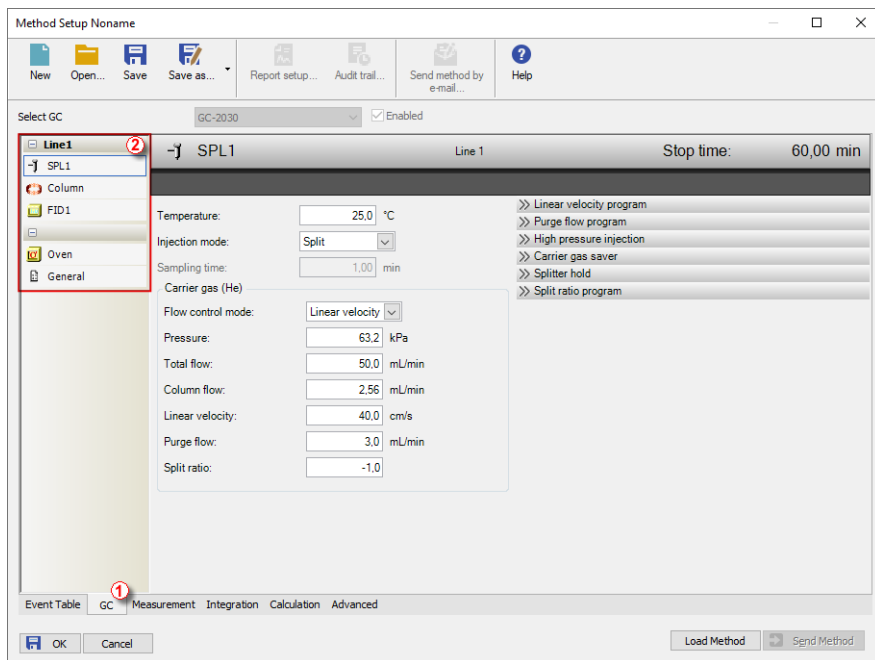


Fig 11: Method Setup - GC

**Note:** Press the **F1** key to display the **Nexis GC-2030 help** with detailed description of the dialog.

From **GC tab** ① you can set all parameters for individual subcomponents (detector/s, oven, inlet...) of instrument configuration.

For advanced setting of all other parameters use all tabs ② on the left side of the window in GC tab.

If there is configured any autosampler of AOC-20 family its parameters are about to set on **GC tab** in its respective section.

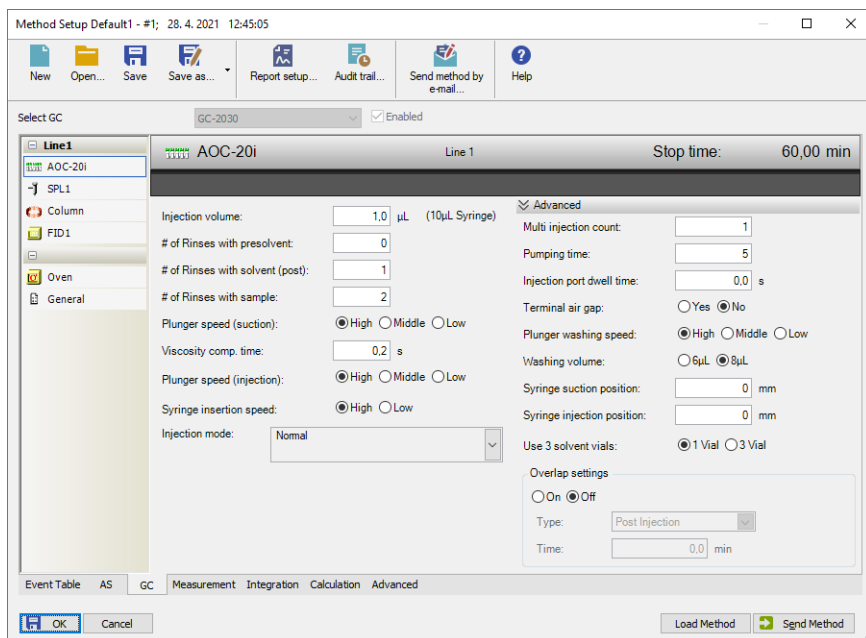


Fig 12: Method Setup - GC - AOC autosampler

**Note:** Actual parameters downloaded from GC are used for new method or method adaptation instead of default parameters.

**Note:** For common analysis it is recommended to relate Oven temperature program via item *Link oven program and acquisition time* otherwise duration of the acquisition is governed by the item *Stop time* in the detector section.

If *Carrier Gas Saver* item is set *On* in the used method it is consequently required to trigger *Start Prep Run* manually by pushing *Prep Run* button above display of the GC or by some external contact. Any of these will transfer the GC to *Ready* state which has to be reached prior actual analysis. If some external contact is about to be used the *Start Prep Run* has to be set as *External* in *General* section of the method. Besides that, it is necessary to have correctly set *Relays* in the "*Module configuration dialog*" on page 8 in the [System Configuration](#). Refer to images below.



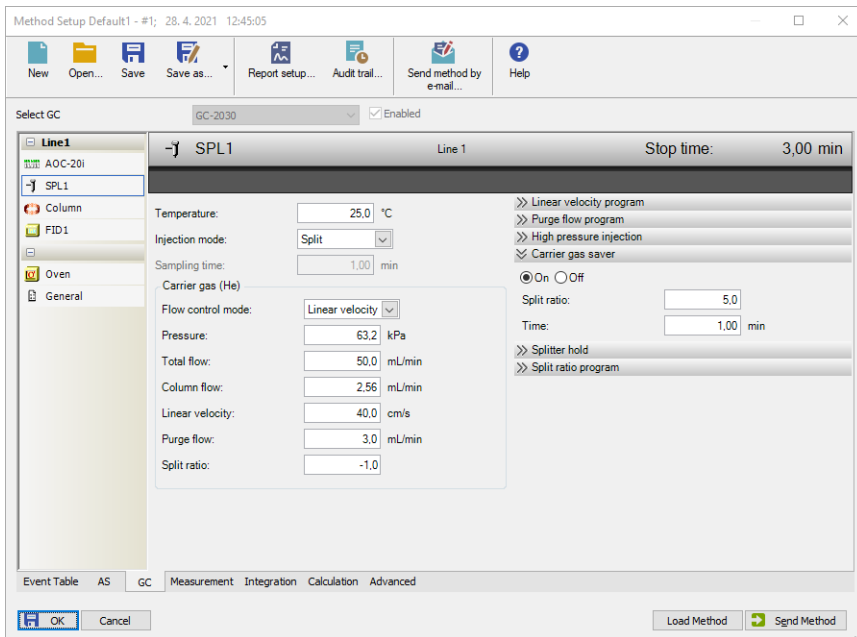


Fig 13: Method Setup - GC - Gas Saver

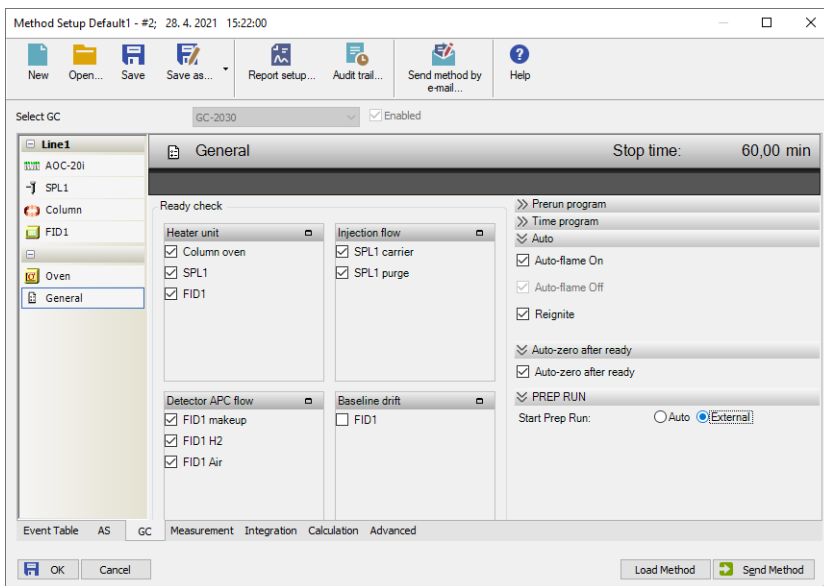


Fig 14: Method Setup - GC - External Prep Run

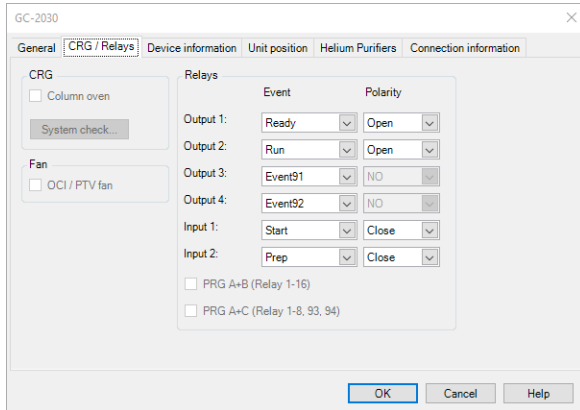


Fig 15: Module configuration - CRG Relays

## 4.2 Device Monitor

The **Device Monitor** window can be opened by the *Device Monitor* command from the *Analysis* menu or using the **Device Monitor** icon in the **Instrument** window. You may use icon for accessing *Device Monitor* from all **Clarity - Shimadzu Edition** windows. This window is for acquiring measured values or control information from instruments so that each instrument status can be monitored.

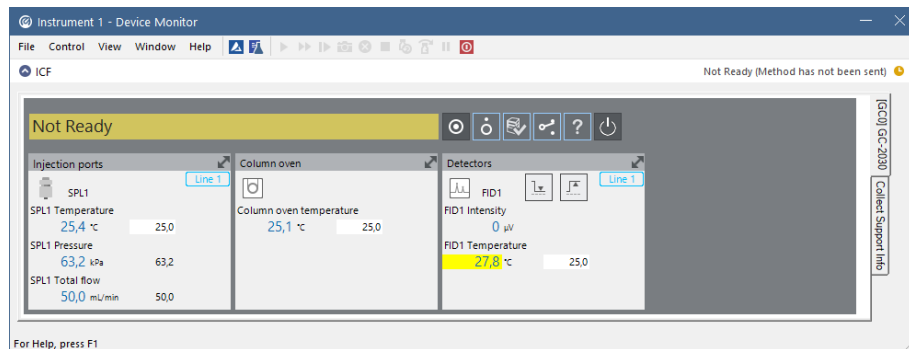


Fig 16: Device Monitor

- Note:** Press the *F1* key to display the **Nexis GC-2030 help** with detailed description of the dialog.
- Note:** Tabs on right side of the *Device Monitor* allowing setting collection of diagnostic information are displayed only when **Clarity - Shimadzu Edition** is started under Administrator Windows account. For other Windows accounts, when running **Clarity - Shimadzu Edition**, there are displayed fewer tabs on the right side of the *Device Monitor*.
- Note:** The *Shutdown* command works as expected only if item *Turn OFF GC on Shutdown* in the "**Nexis GC-2030 Setup**" on page 6 dialog of the **System Configuration** is checked. If such commands were applied there will be applied setting defined in section *System Off parameters* from the tab *General* of the "*Module configuration dialog*" on page 8 dialog.
- Note:** Some errors cannot be cleared using *Device Monitor* and have to be cleared via manual commands using display of the GC.

## 5 Troubleshooting

When the solution for some problem cannot be discovered easily, the recording of communication between **Clarity - Shimadzu Edition** and *Shimadzu Nexis GC-2030* control module can significantly help the **DataApex** support to discover the cause of the problem. The created \*.TXT files will greatly help in diagnosis of unrecognized errors and problems.

The recording can be enabled by adding or amending the LOGGING.INI file in the **Clarity - Shimadzu Edition** installation directory (C:\CLARITYSHIMADZU\CFG by default). The file can be edited in any text editor (e.g. Notepad). Following section should be edited:

```
[Log]
echo = ON
filename = log_%D.txt
reset = OFF
; Sections List:
AuditTrail = ON
BadTrace = ON
CommandLine = ON
Acquisit = ON
AgilentICF = ON
SST = OFF
Internet = OFF
FractionCollector = OFF
```

---

**Note:** %D (or %d) in the filename parameter means that the log will be created separately for each day. The *reset = OFF* parameter disables deleting the content of the log each time the station is started during the same day.

In case you cannot establish communication with Agilent instruments, please review the following issues:

### **Check the network connection using the Ping command**

The problem in communication between **Clarity - Shimadzu Edition** and Shimadzu Nexis GC-2030 may be caused by wrong network configuration, firewall preventing the connection, etc. Run the command line in Windows (for example by pressing the **Windows key** together with the **R** key, in the displayed **Run** window type *cmd* and press *Enter*). In the command line type `ping <ip-address-of-instrument>` and press *Enter*. The *IP Address* is the same you entered during the configuration.

## 5.1 Specific Problems

### Clarity - Shimadzu Edition can't be run and it displays "Agilent ICF is not installed correctly." message.

**Cause:** The cause of the problem is that the Agilent ICF has a different version than expected by Clarity - Shimadzu Edition. It can typically happen when other software also using Agilent ICF decides to reinstall it. Thus next time Clarity - Shimadzu Edition expects different version than is installed.

**Solution:** Solution is to reinstall Agilent ICF during Clarity - Shimadzu Edition installation. Follow steps described in the chapter "**Installation procedure**" on pg 3.

### Headspace autosamplers have not been tested.

**Cause:** There have been implemented *Sequence Mode* and *Enable Sample Overlap* functionality but their usage with Headspace autosamplers has not been tested yet.

**Solution:** We are working to fix this situation.

### Print of *Injection Control* is not functional.

**Cause:** Agilent ICF is incompatible with some Clarity - Shimadzu Edition printing procedures.

**Solution:** Method parameters of autosampler control are printed together with another GC control method parameters using *Instrument Control* item within *Method* section in *Report Setup* dialog.

### ICF problems during installation or operation.

**Cause:** The cause of the problem might be that *Microsoft .NET Framework* is not enabled. Agilent ICF requires *Microsoft .NET Framework* enabled for its function.

**Solution:** Check if *Microsoft .NET Framework* is enabled in *Turn Windows features on or off* dialog. If *Microsoft .NET Framework* is not enabled enable it. *Turn Windows features on or off* dialog is accessible in *Control Panel* window under section *Programs* in its subsection *Programs and Features*. The *Microsoft .NET Framework* related items are disabled by default in some *Windows* versions.

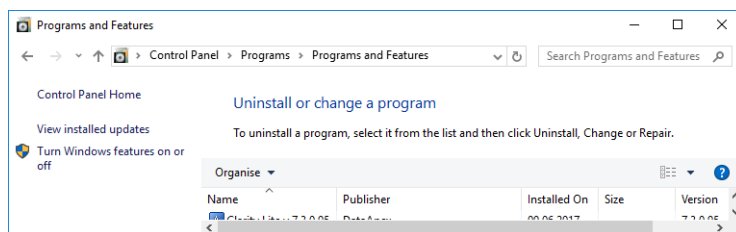


Fig 17: Location of *Turn Windows features on or off* in *Windows 10*

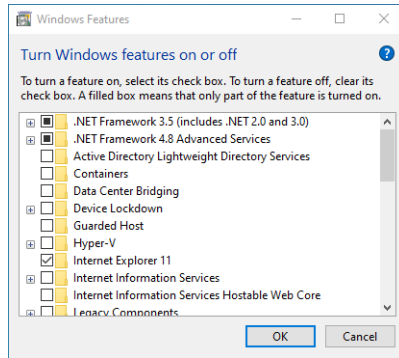


Fig 18: Turn Windows features on or off - Windows 10